


CK520A: 4-in-1 OSLT Calibration Kit, DC to 26.5 GHz, Type-3.5 mm (m) 50 Ohm

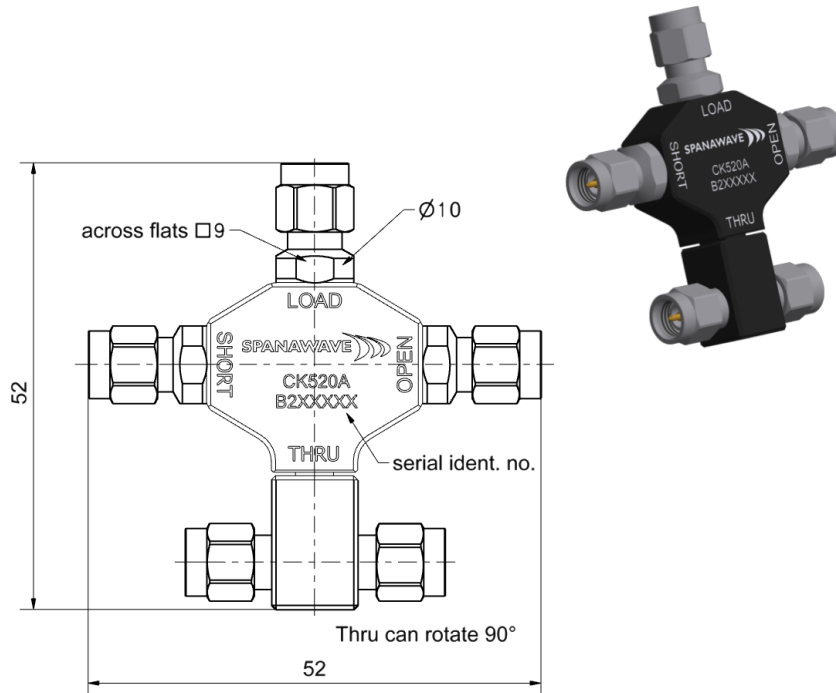

Interface

According to 3.5 mm (m)
Mechanically compatible with 2.92 mm and SMA

Contents and Documentation

This kit is delivered with

- **Standard Definitions Card**
Printed Standard Definitions that can be used on nearly all Vector Network Analyzers
- **Test Results Documentation**
- **Hard Shell Case**

Material and plating

Connector parts

Center conductor
Outer conductor
Coupling nut
Body
Dielectric
Substrate

Material

Beryllium copper
Stainless steel
Stainless steel
Aluminum
PS
Al₂O₃

Plating

Gold, min. 1.27 µm, over nickel
Passivated
Passivated
black anodized

CK520A: 4-in-1 OSLT Calibration Kit, DC to 26.5 GHz, Type-3.5 mm (m) 50 Ohm

Electrical data

| | |
|---------------------------------------|---|
| Frequency range | DC to 26.5 GHz |
| Thru | |
| Return loss | ≥ 34 dB, DC to 4 GHz ≥ 32 dB, 4 GHz to 8 GHz ≥ 30 dB, 8 GHz to 26.5 GHz |
| Open | |
| Error from nominal phase ¹ | $\leq 1.0^\circ$, DC to 4 GHz $\leq 2.0^\circ$, 4 GHz to 8 GHz $\leq 3.0^\circ$, 8 GHz to 26.5 GHz |
| Short | |
| Error from nominal phase ² | $\leq 1.0^\circ$, DC to 4 GHz $\leq 2.0^\circ$, 4 GHz to 8 GHz $\leq 3.0^\circ$, 8 GHz to 26.5 GHz |
| Load | |
| Return loss | ≥ 40.0 dB, DC to 4 GHz ≥ 35.0 dB, 4 GHz to 8 GHz ≥ 30.0 dB, 8 GHz to 26.5 GHz |
| DC Resistance | $50 \Omega \pm 0.5 \Omega$ |
| Power handling | ≤ 0.5 W |

¹ The nominal phase is defined by the Offset Delay, the Offset Loss and the Fringing Capacitances.

² The nominal phase is defined by the Offset Delay, the Offset Loss and the Short Inductance.

Mechanical data

| | |
|--------------------|--------------------|
| Mating cycles | ≥ 500 |
| Maximum torque | 1.70 Nm |
| Recommended torque | 0.90 Nm |
| Gauge | 0.00 mm to 0.08 mm |

General standard definitions

For proper operation the vector network analyzer (VNA) needs a model describing the electrical behavior of this calibration standard. The different models, units, and terms used will depend on the VNA type and they will have to be entered into the VNA. All values are based on typical geometry and plating.

Thru

| | |
|-------------------------------------|--------------------------------|
| Offset Z_0 / Impedance / Z_0 | 50 Ω |
| Offset Delay | 84.058 ps |
| Length (electrical) / Offset Length | 25.20 mm |
| Offset Loss | 2.51 G Ω /s |
| Loss | 0.0183 dB/ $\sqrt{\text{GHz}}$ |
| Line Loss @ 1GHz | 0.0007 dB/mm |

Open

| | |
|-------------------------------------|--|
| Offset Z_0 / Impedance / Z_0 | 50 Ω |
| Offset Delay | 33.356 ps |
| Length (electrical) / Offset Length | 10.00 mm |
| Offset Loss | 2.20 G Ω /s |
| Loss | 0.0127 dB/ $\sqrt{\text{GHz}}$ |
| Fringing Capacitances | $C_0 = -17.000 \times 10^{-15}$ F / -17.000 fF $C_1 = -2000.0 \times 10^{-27}$ F/Hz / -2.0000 fF /GHz $C_2 = 147.00 \times 10^{-36}$ F/Hz ² / 0.1470 fF /GHz ² $C_3 = -3.0000 \times 10^{-45}$ F/Hz ³ / -0.0030 fF /GHz ³ |

CK520A: 4-in-1 OSLT Calibration Kit, DC to 26.5 GHz, Type-3.5 mm (m) 50 Ohm

Short

| | |
|-------------------------------------|--|
| Offset Z_0 / Impedance / Z_0 | 50 Ω |
| Offset Delay | 33.356 ps |
| Length (electrical) / Offset Length | 10.00 mm |
| Offset Loss | 2.36 G Ω /s |
| Loss | 0.0127 dB/ $\sqrt{\text{GHz}}$ |
| Short Inductance | $L_0 = -39.000 \times 10^{-12} \text{ H} \quad / \quad -39.000 \text{ pH}$ $L_1 = 2200.0 \times 10^{-24} \text{ H/Hz} \quad / \quad 2.2000 \text{ pH /GHz}$ $L_2 = -150.00 \times 10^{-33} \text{ H/Hz}^2 \quad / \quad -0.1500 \text{ pH /GHz}^2$ $L_3 = 3.0000 \times 10^{-42} \text{ H/Hz}^3 \quad / \quad 0.0030 \text{ pH /GHz}^3$ |

Load

| | |
|-------------------------------------|--------------------------------|
| Offset Z_0 / Impedance / Z_0 | 50 Ω |
| Offset Delay | 0.0000 ps |
| Length (electrical) / Offset Length | 0.000 mm |
| Offset Loss | 0.00 G Ω /s |
| Loss | 0.0000 dB/ $\sqrt{\text{GHz}}$ |

Environmental data

| | |
|---|------------------|
| Operating temperature range ³ | +20 °C to +26 °C |
| Rated temperature range of use ⁴ | 0 °C to +50 °C |
| Storage temperature range | -40 °C to +85 °C |
| RoHS | compliant |

³ Temperature range over which these specifications are valid.

⁴ This range is underneath and above the operating temperature range, within the calibration kit is fully functional and could be used without damage.

Includes

Standard delivery for this kit includes Test Results. The documentation issued reports which quantities were tested individually, traceable to national / international standards. Model based standard definitions of the calibration standards are reported in Agilent / Keysight, Rohde & Schwarz and Anritsu compatible VNA format.

Calibration interval

| | |
|----------------|-----------|
| Recommendation | 12 months |
|----------------|-----------|

Packing

| | |
|----------|-----------|
| Standard | 1 per bag |
| Weight | 1.35 oz. |

While the information has been carefully compiled to the best of our knowledge, nothing is intended as representation or warranty on our part and no statement herein shall be construed as recommendation to infringe existing patents. In the effort to improve our products, we reserve the right to make changes judged to be necessary.